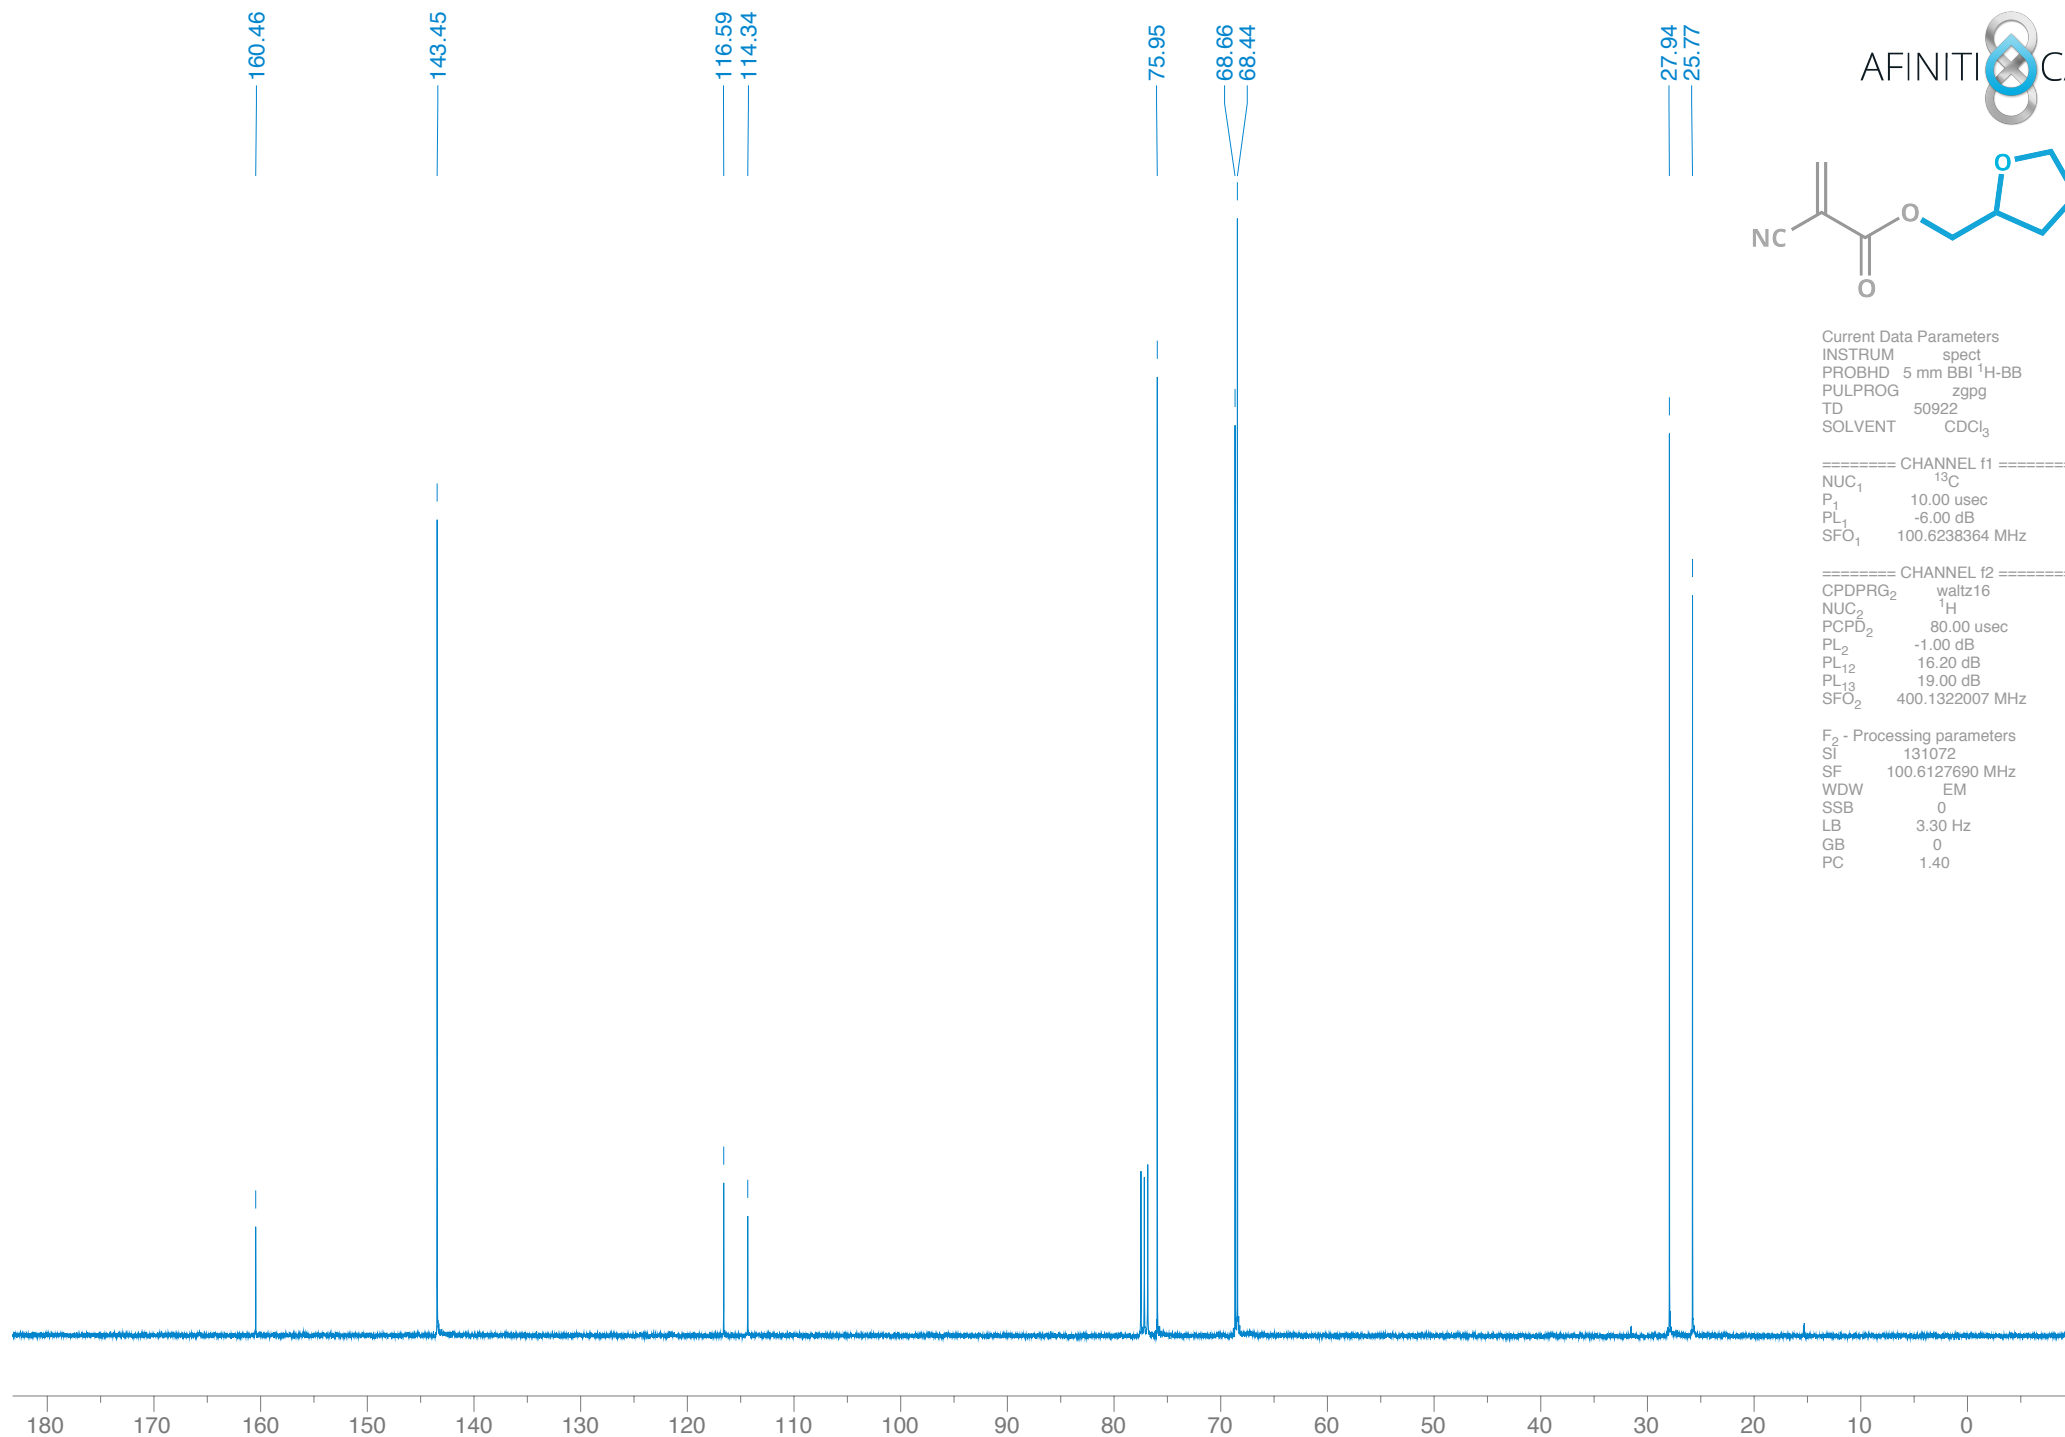


Current Data Parameters
INSTRUM spect
PROBHD 5 mm BBI ¹H-BB
PULPROG zgpg
TD 50922
SOLVENT CDCl₃

===== CHANNEL f1 =====
NUC₁ ¹³C
P₁ 10.00 usec
PL₁ -6.00 dB
SFO₁ 100.6238364 MHz

===== CHANNEL f2 =====
CPDPRG₂ waltz16
NUC₂ ¹H
PCPD₂ 80.00 usec
PL₂ -1.00 dB
PL₁₂ 16.20 dB
PL₁₃ 19.00 dB
SFO₂ 400.1322007 MHz

F₂ - Processing parameters
SI 131072
SF 100.6127690 MHz
WDW EM
SSB 0
LB 3.30 Hz
GB 0
PC 1.40